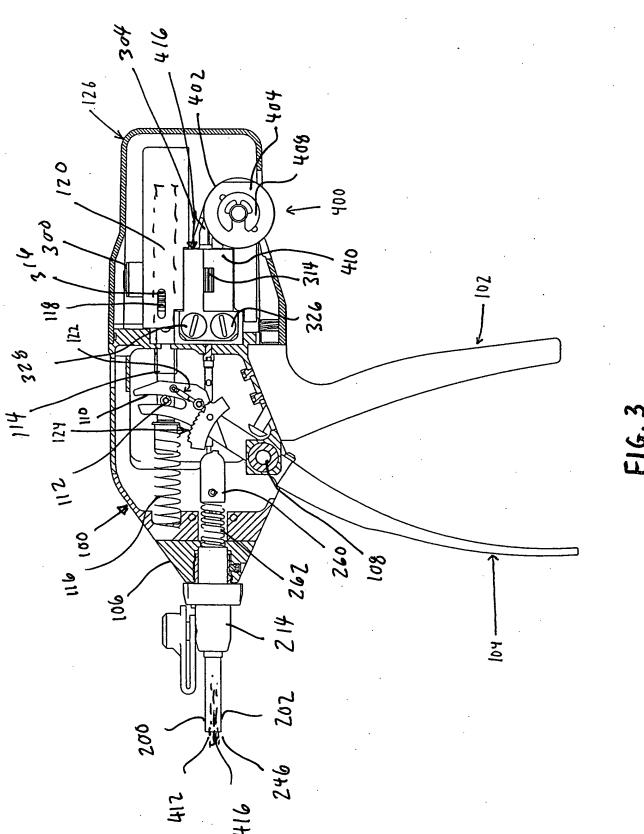
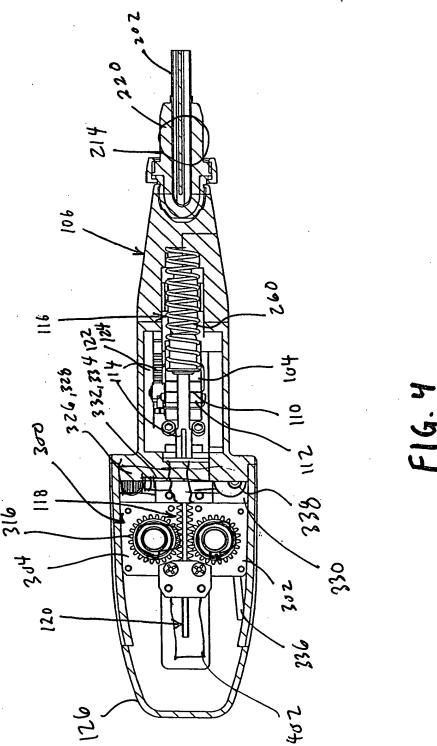


F G





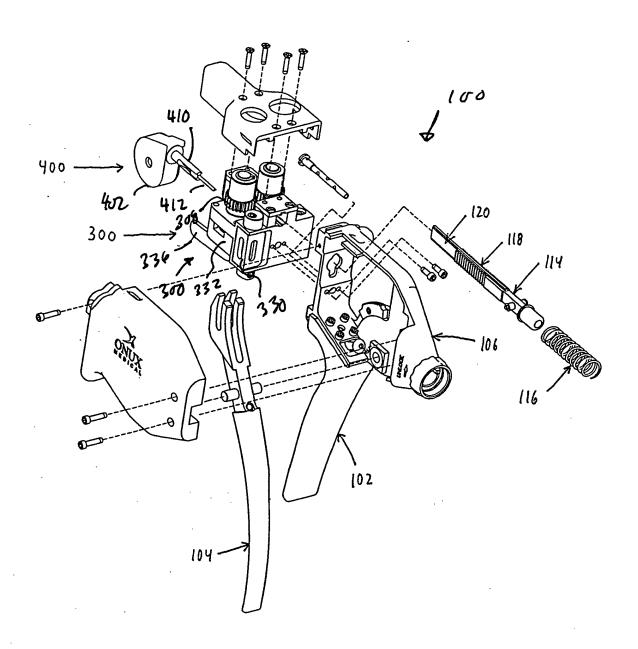
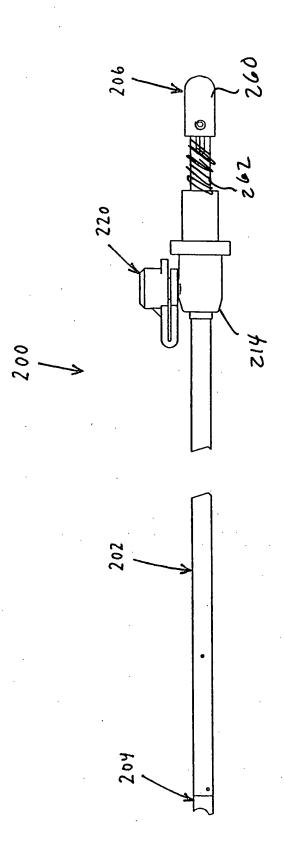
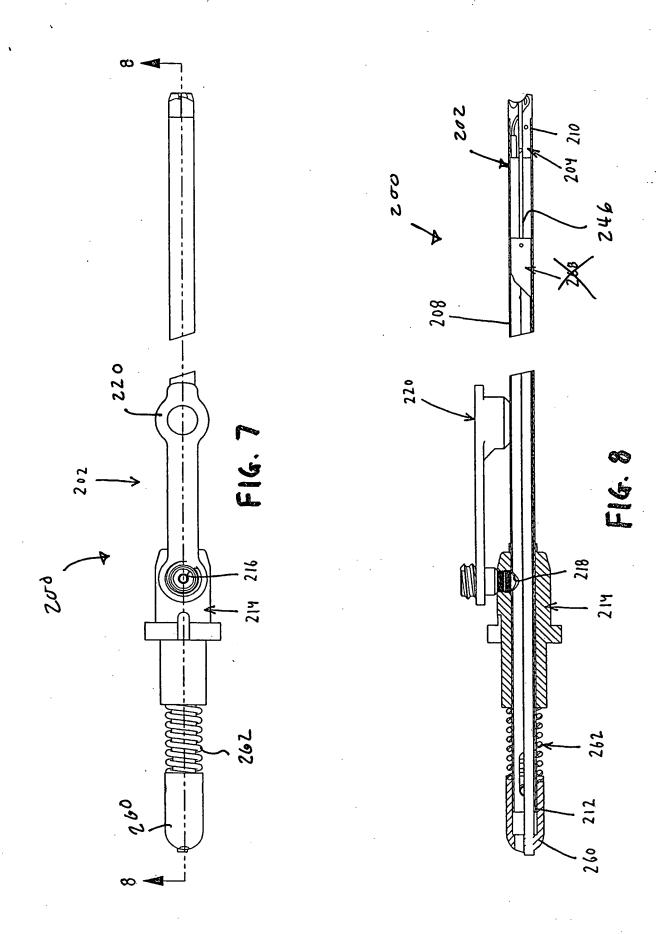


FIG. 5






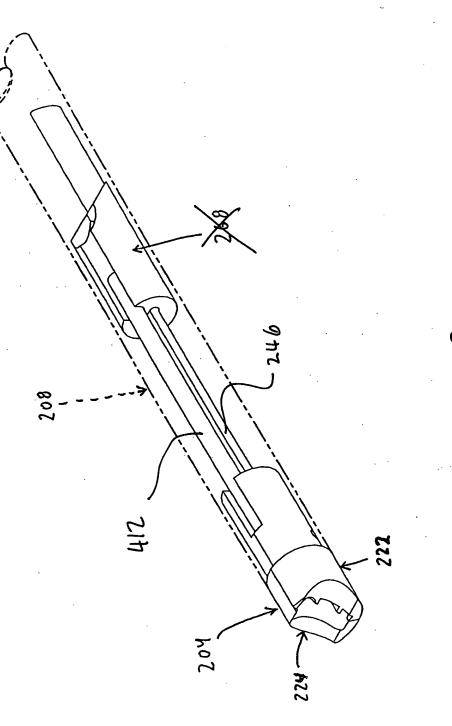


FIG. 9

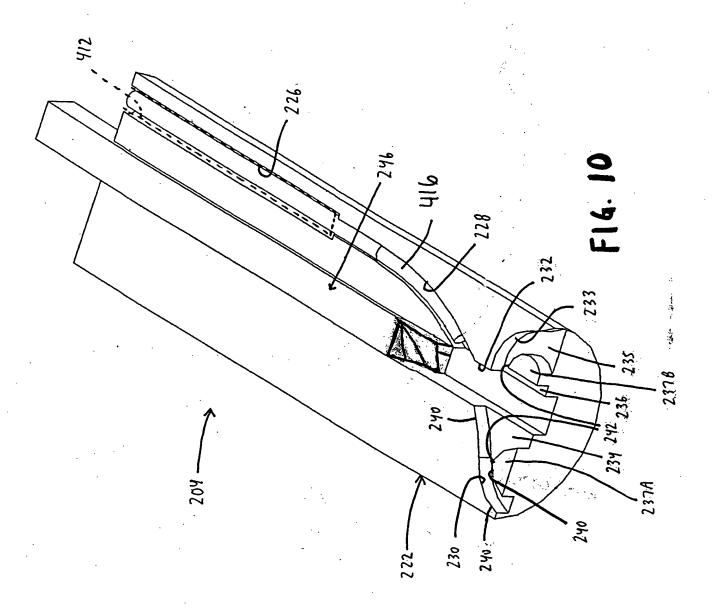

Serial No.: 10/737,197

For: SURGICAL SUTURING INSTRUMENT AND METHOD OF USE
Applicant: Frederic P. Field et al.
ANNOTATED SHEET




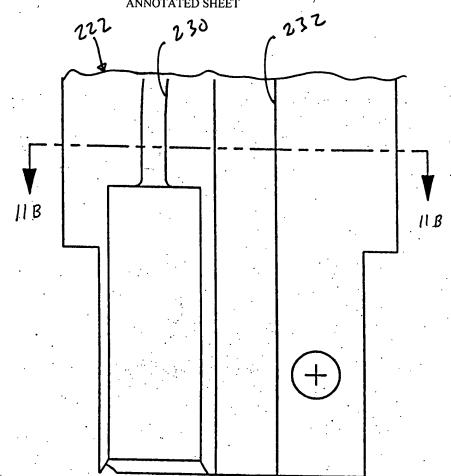


FIG. II A

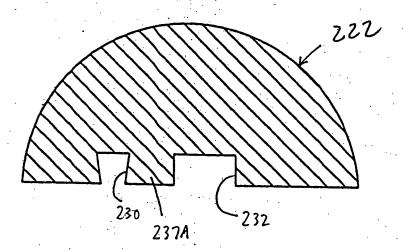


F14. 11B

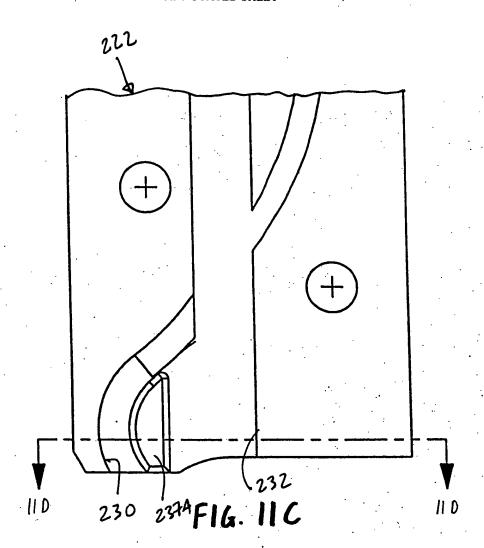


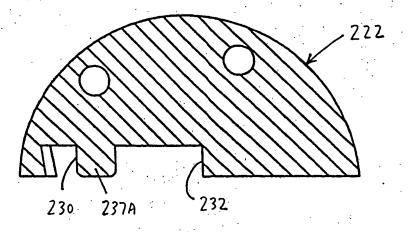

F14. 110

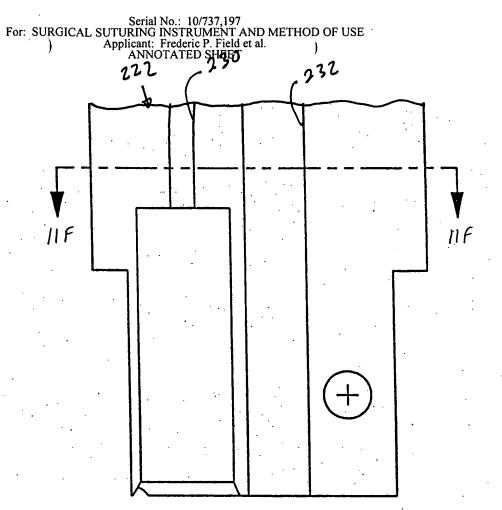


F16.11E

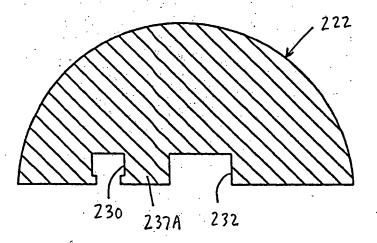


F16. 11 F


Serial No.: 10/737,197

For: SURGICAL SUTURING INSTRUMENT AND METHOD OF USE Applicant: Frederic P. Field et al. ANNOTATED SHEET

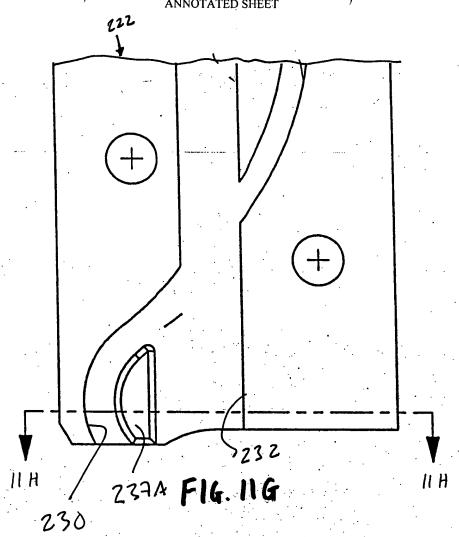


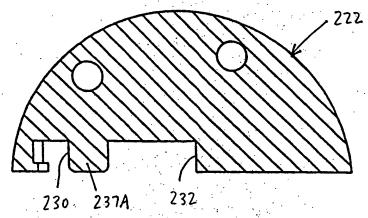

F16. 11 H

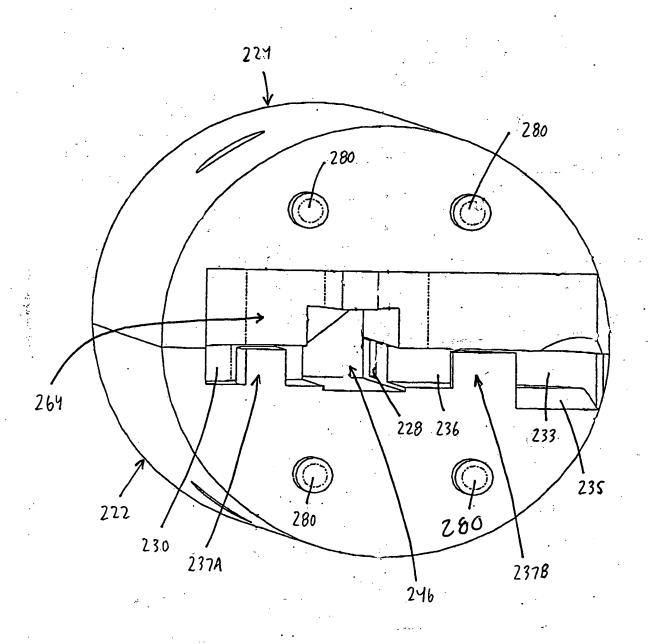

F16. 11 I

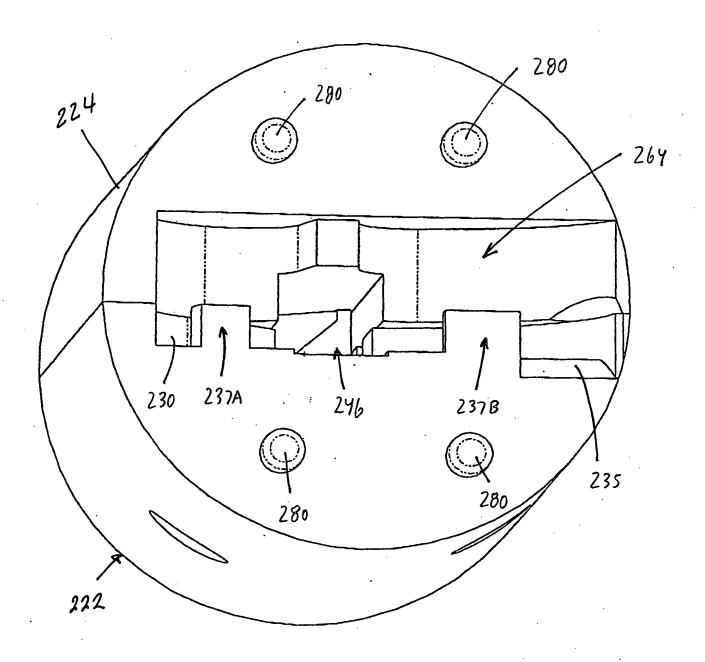

F16. 11 J

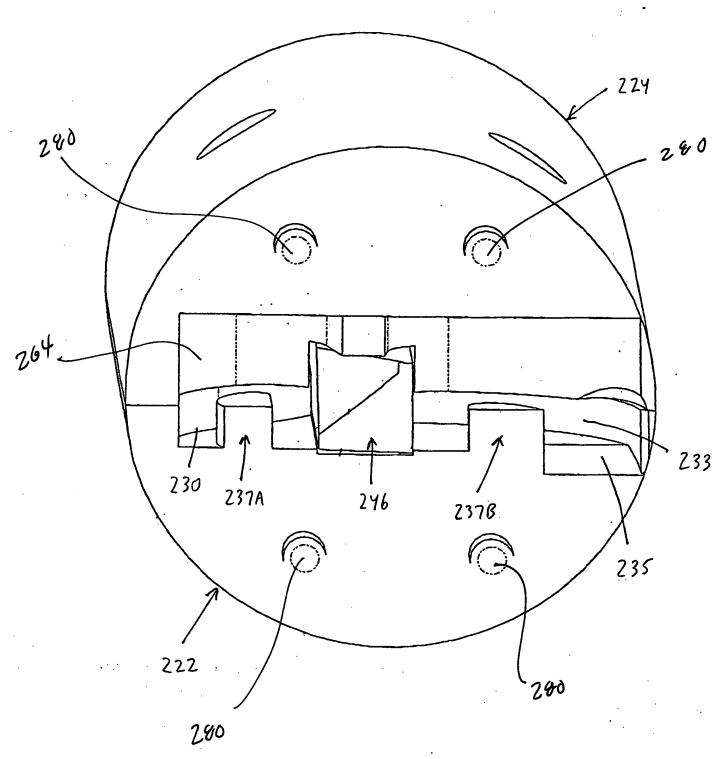
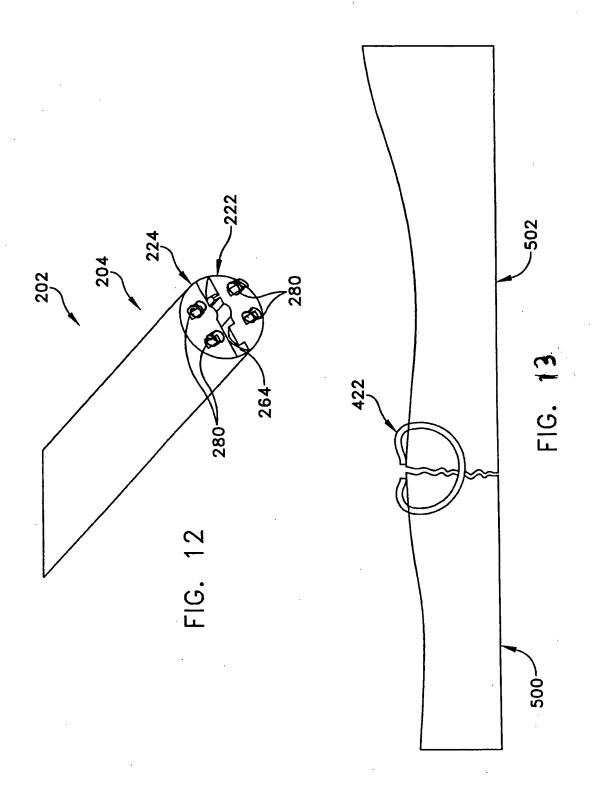
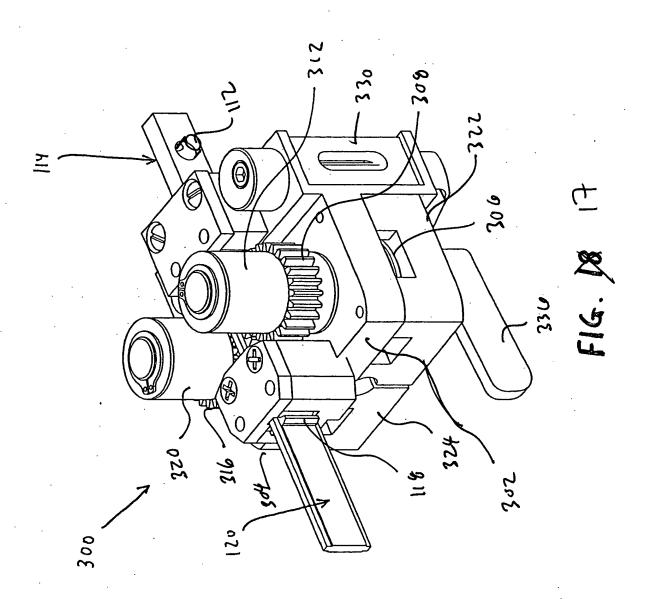
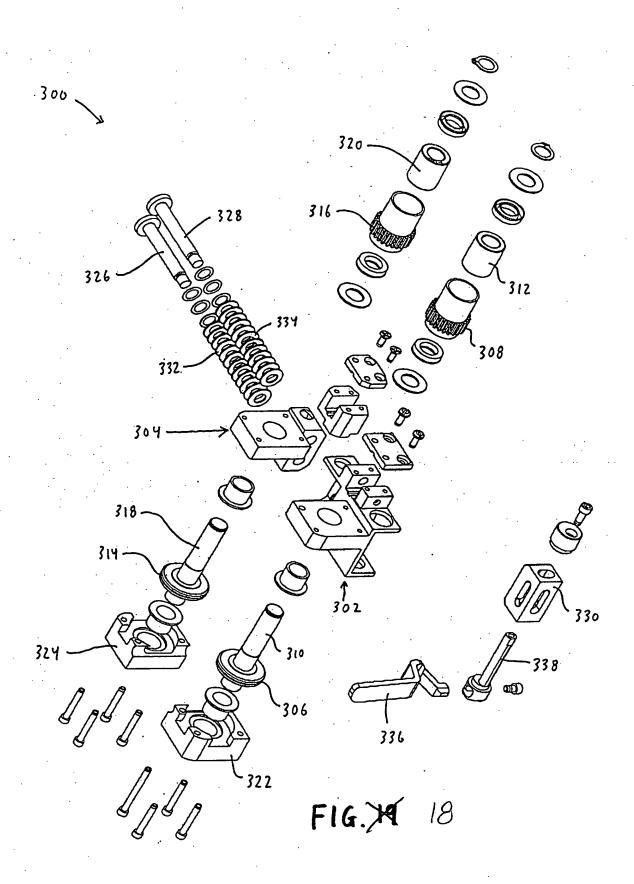
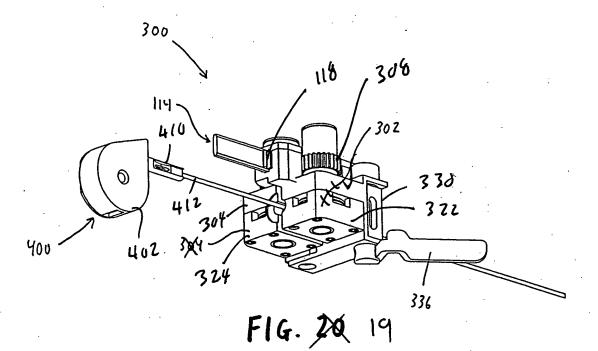


FIG. IIK









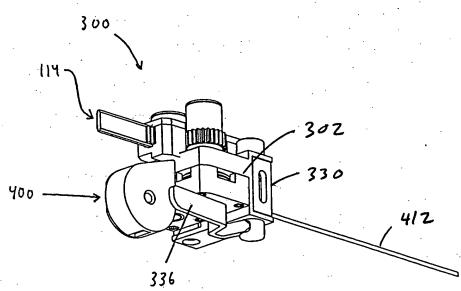
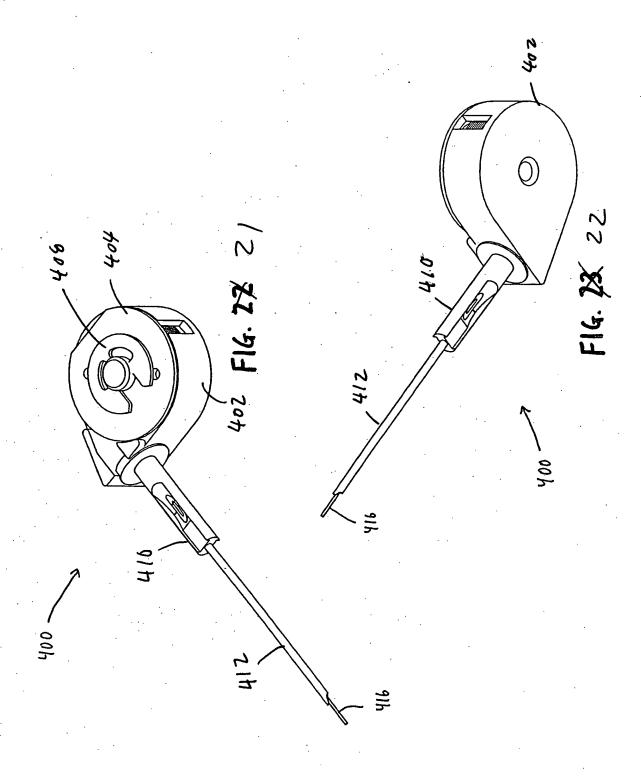
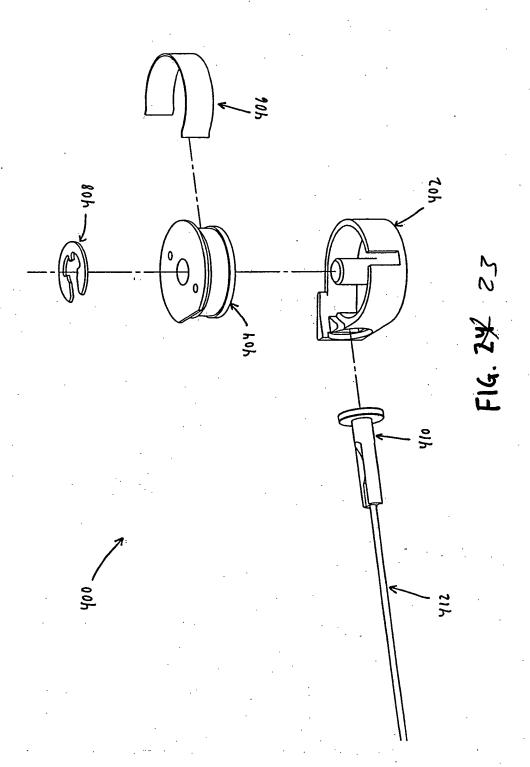
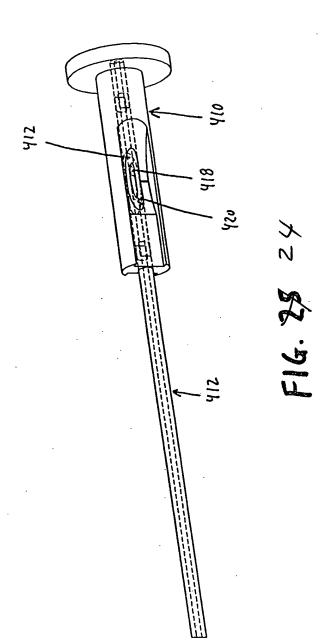
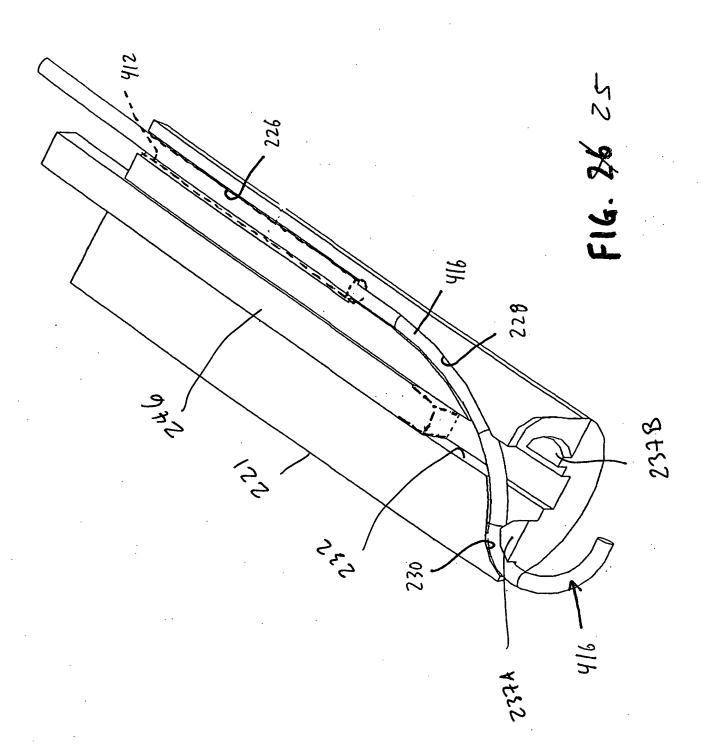



FIG. 24 20













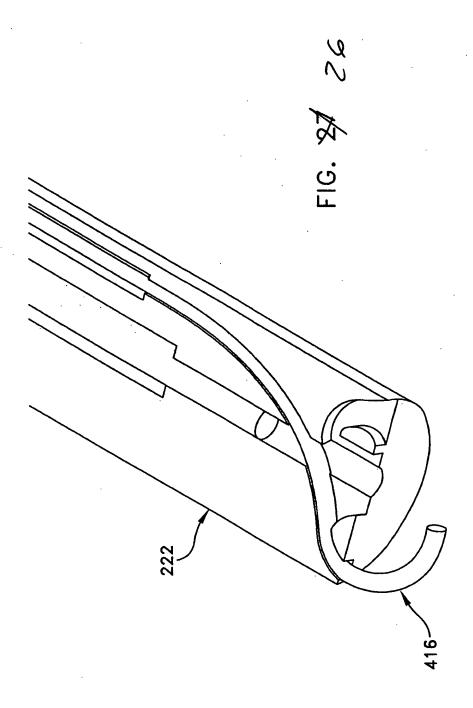


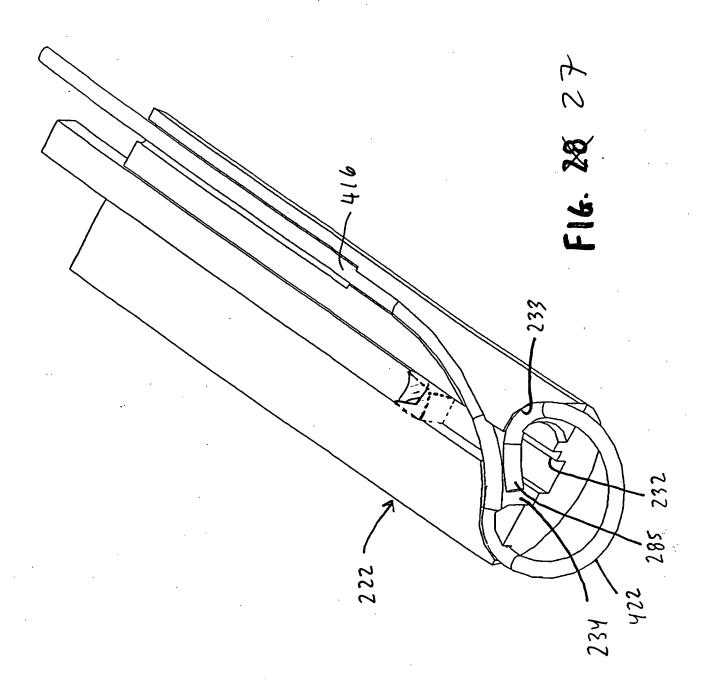


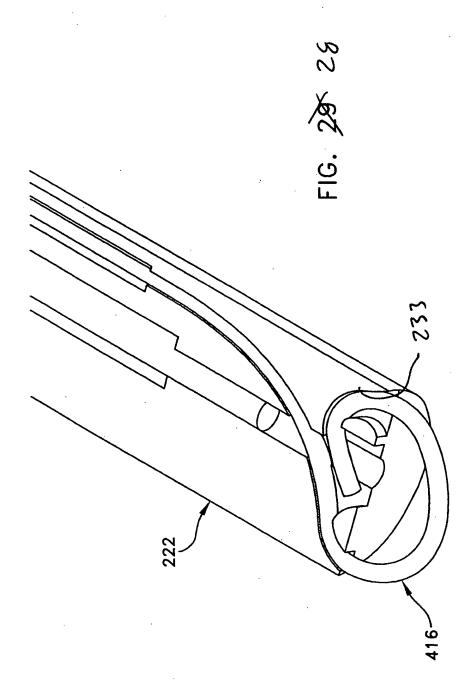

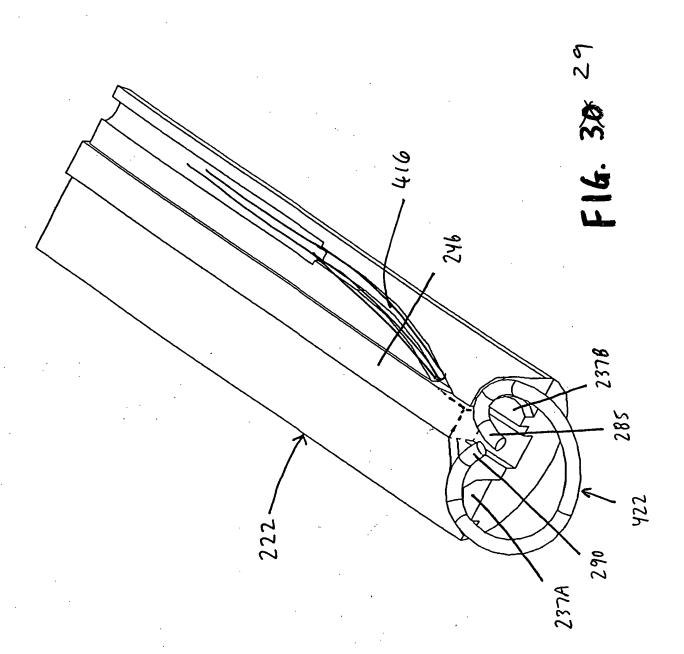

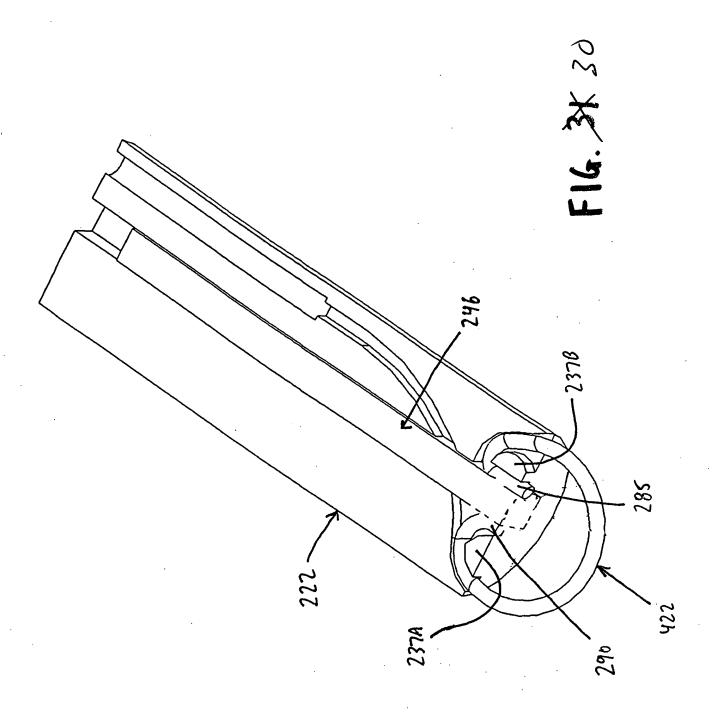

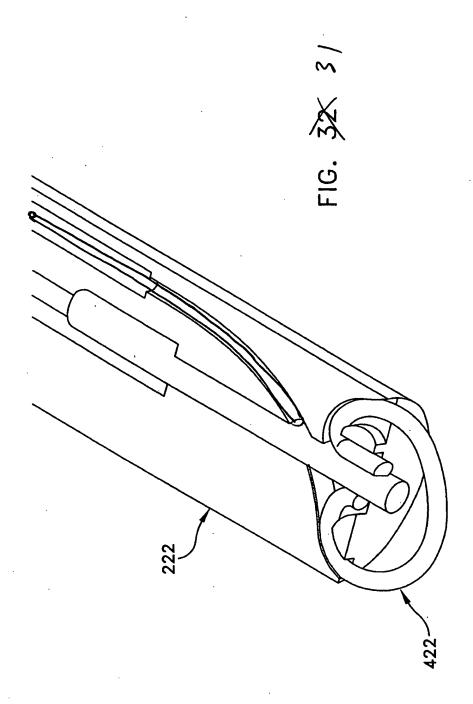

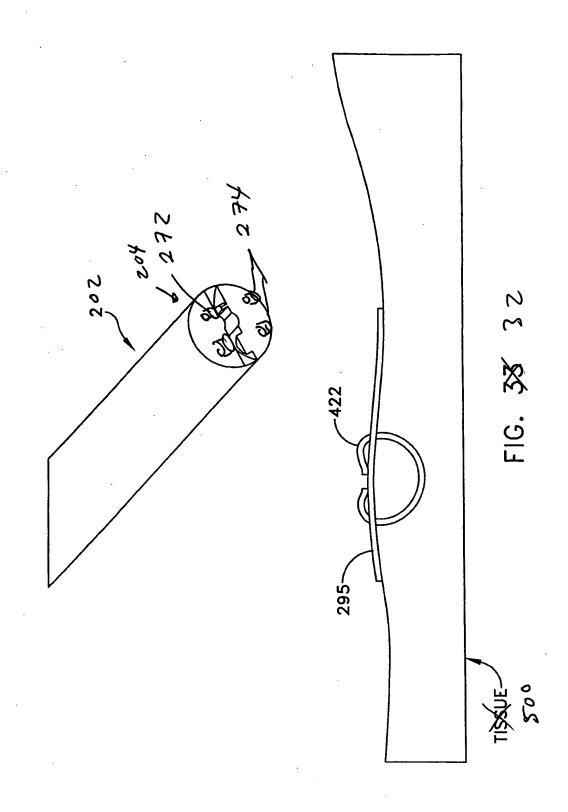

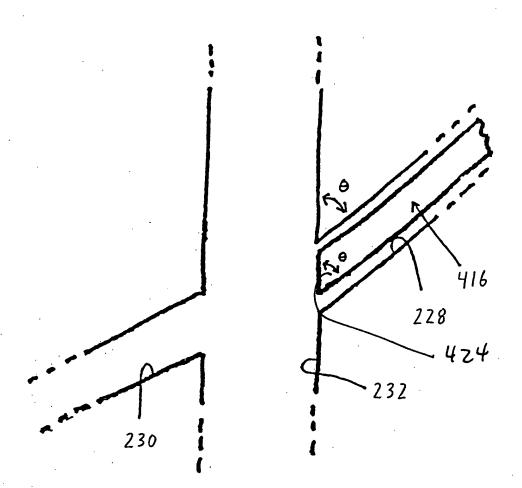


FIG. 35 33


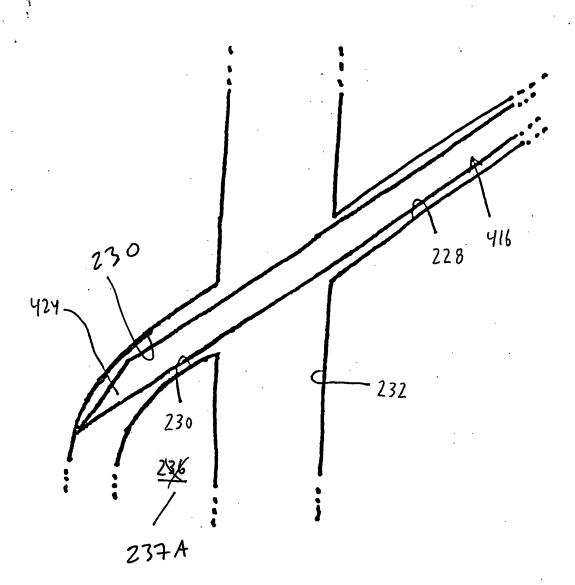


FIG. 36 34

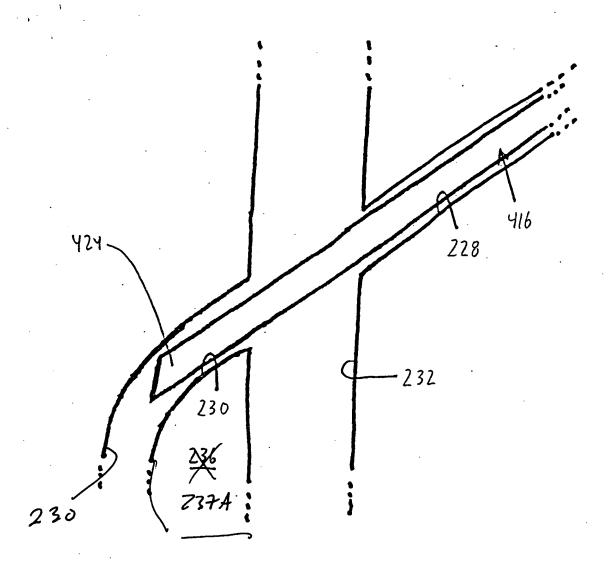

F14.37 35